

## Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE <b>bpc-157</b>	RECEIVED DATE <b>Mar 30, 2026</b>	ANALYSIS DATE <b>Apr 01, 2026</b>	REPORT GENERATED <b>Apr 02, 2026</b>
STRENGTH	<b>10mg</b>	MANUFACTURER	<b>PepticoAminos</b>
BATCH NUMBER	<b>PC-BP10-0406F</b>	LAB CODE	<b>458-1</b>
CLIENT	<b>www.pepticoaminos.net</b>		

## SAMPLE INFORMATION

**bpc-157****10MG**FORM **White powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-BP10-0406F**CAP / CRIMP COLOR **blue / Silver**RECEIVED DATE **Mar 30, 2026**

SAMPLE IMAGE


## ANALYTICAL SUMMARY

IDENTITY	<b>BPC-157</b>
PURITY	<b>99.672%</b>
QUANTITY	<b>10.45mg</b>
BATCH	<b>PC-BP10-0406F</b>
MANUFACTURER	<b>PepticoAminos</b>

# RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm

Sample ID: bpc-157  
Report ID: 2024-02-01-04001  
Method: RP-HPLC-UV Method For Peptide Analysis  
Detector: UV 220 nm | Runtime: 12.0 min

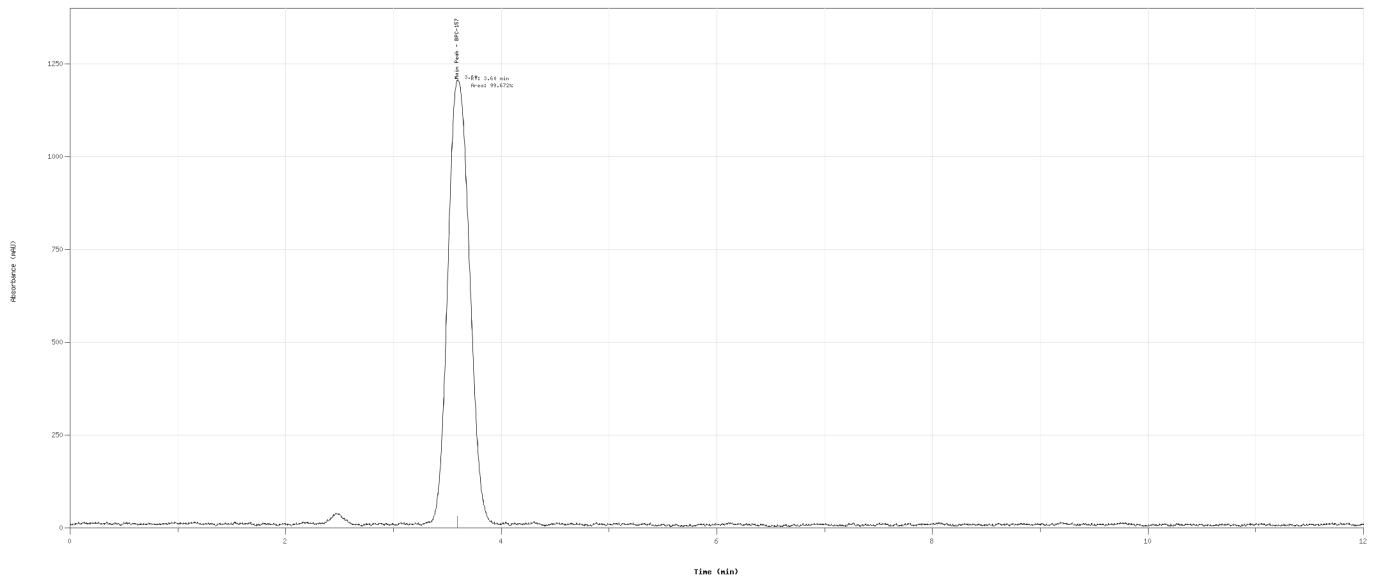

## METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	95%	5%
2min	95%	5%
10min	8%	92%
12min	8%	92%

## TECHNICAL NOTE

Gradient RP-HPLC-UV screening method with UV detection at 220 nm. Runtime 12.0 min.


## COMMENTS

The analytical evaluation confirms the identity of the sample. Purity is within acceptable limits, with only trace levels of related compounds detected. Overall profile is consistent with established reference standards.

## LC-MS MASS SPECTRUM

Sample: BPC-137  
Report ID: 2024-2025-004861  
Reference MW: 1452.5 Da  
Ionization: ESI+

Acquisition: LC-MS  
Profile: Mass Centroid

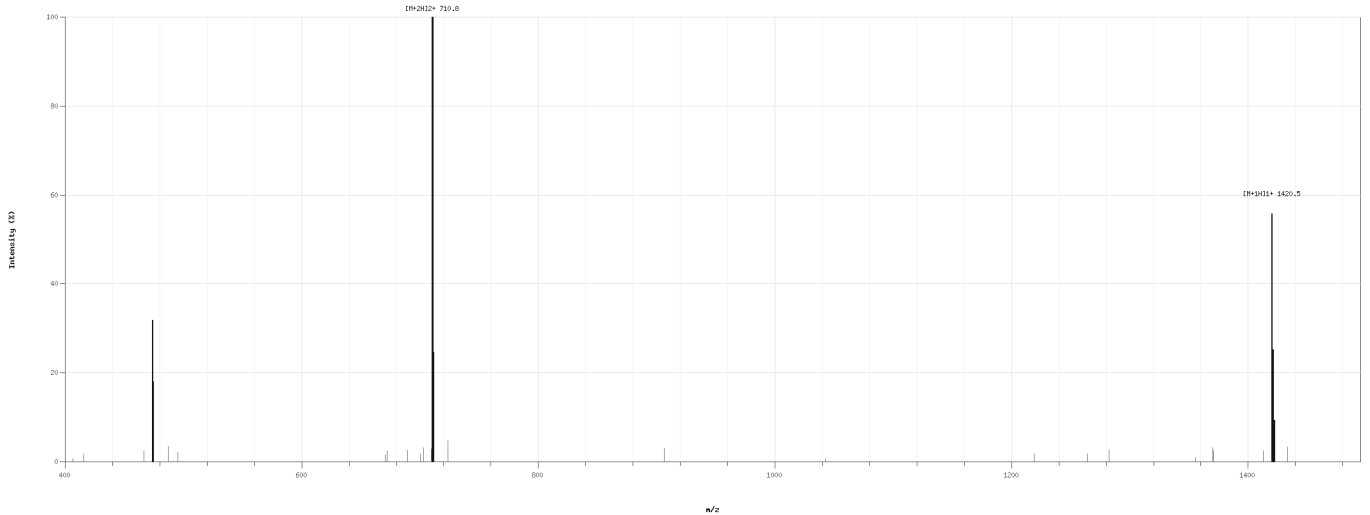

Charge-state distribution and isotope clustering consistent with the analyzed sample.

## ANALYSIS & METHODOLOGY

### STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

HPLC-UV: High-Performance Liquid Chromatography with Ultraviolet detection. Additional testing includes bioburden screening, endotoxin analysis and heavy metals assessment.

### BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Total Aerobic Microbial Count</b> USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 1000
<b>Total Yeast and Mold Count</b> USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 100

### ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Bacterial Endotoxin</b> USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	< 0.001	EU/mg	> 0.5

### HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Arsenic</b> Elemental Impurities Screening	Not detected	ppm	>= 1.5
<b>Cadmium</b> Elemental Impurities Screening	Not detected	ppm	>= 0.5
<b>Cobalt</b> Elemental Impurities Screening	Not detected	ppm	>= 25
<b>Lead</b> Elemental Impurities Screening	Not detected	ppm	>= 1.5

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Nickel</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>
<b>Quicksilver</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 1.5</b>
<b>Vanadium</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>

## TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

## COMPOUND REFERENCE

PARAMETER	BPC-157
<b>PUBCHEM CID</b>	9941957
<b>CAS</b>	137525-51-0
<b>MOLECULAR FORMULA</b>	C62H98N16O22
<b>MOLECULAR WEIGHT</b>	1419.5 g/mol

## METHOD SPECIFICATION

PARAMETER	RP-HPLC-UV METHOD FOR PEPTIDE ANALYSIS
<b>ANALYTICAL MODE</b>	Purity assessment of peptide sample by RP-HPLC-UV
<b>COLUMN</b>	C18 peptide column, 150 x 4.6 mm equivalent
<b>MOBILE PHASE A</b>	Water + 0.1% TFA
<b>MOBILE PHASE B</b>	Acetonitrile + 0.1% TFA
<b>FLOW RATE</b>	1.0 mL/min
<b>DETECTION</b>	UV 220 nm
<b>INJECTION VOLUME</b>	10 uL
<b>RUNTIME</b>	12.0 min
<b>SAMPLE DILUENT</b>	Water/acetonitrile compatible diluent
<b>SAMPLE PREPARATION</b>	Diluted to working concentration and filtered/clarified

## INSTRUMENT PLATFORM

PARAMETER	STANDARD HPLC-UV PLATFORM
<b>SYSTEM TYPE</b>	Analytical HPLC system
<b>DETECTOR</b>	UV/VIS detector
<b>ACQUISITION</b>	Chromatographic acquisition and integration software
<b>REVIEW MODE</b>	Retention-time and response-profile review

PARAMETER	STANDARD HPLC-UV PLATFORM
WORKFLOW NOTE	Used for routine peptide purity and identity screening

## ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
IDENTITY	Retention-time and profile agreement with reference expectations	Chromatographic identity review
PURITY	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
QUANTITY	Measured content reviewed against the declared sample strength	Report-level analytical summary
BIOBURDEN	Not detected or within stated reporting limits	Microbial screening table
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

## VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

**Verification URL** [synaptica-labs.com/verify-report/](https://synaptica-labs.com/verify-report/)

**Report ID** SYN-2026-004861

**Verification Key** VK-ZJYC-68E3

SCAN TO VERIFY



## DIGITAL SIGNATURE



**DIGITALLY SIGNED BY:**

**Martin Saar**

Date: 2026.04.02

15:24:46 +02'00'

Director

[info@synaptica-labs.com](mailto:info@synaptica-labs.com)

Analysis date: Apr 01, 2026

Report generated: Apr 02, 2026

Analytical testing performed by Synaptica Analytics -  
Analytical Services Division

Synaptica Analytics  
**SYN-2026-004861**  
Laboratory Analysis Report  
**VK-ZJYC-68E3**

**VERIFY AT**  
[synaptica-labs.com/verify-report/](https://synaptica-labs.com/verify-report/)