

Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE KPV	RECEIVED DATE Mar 12, 2026	ANALYSIS DATE Mar 18, 2026	REPORT GENERATED Mar 19, 2026
STRENGTH	10mg	MANUFACTURER	PepticoAminos
BATCH NUMBER	PC-KP10-1012U	LAB CODE	887-2
CLIENT	www.pepticoaminos.net		

SAMPLE INFORMATION

KPV**10MG**FORM **White powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-KP10-1012U**CAP / CRIMP COLOR **Trasp. Red/Black**RECEIVED DATE **Mar 12, 2026**

SAMPLE IMAGE


ANALYTICAL SUMMARY

IDENTITY	KPV
PURITY	99.732%
QUANTITY	11.32mg
BATCH	PC-KP10-1012U
MANUFACTURER	PepticoAminos

RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm

Sample ID: KPV
Report ID: 2019-2020-004077
Method: RP-HPLC-UV Short Peptide
Detector: UV 220 nm | Runtime: 12.0 min

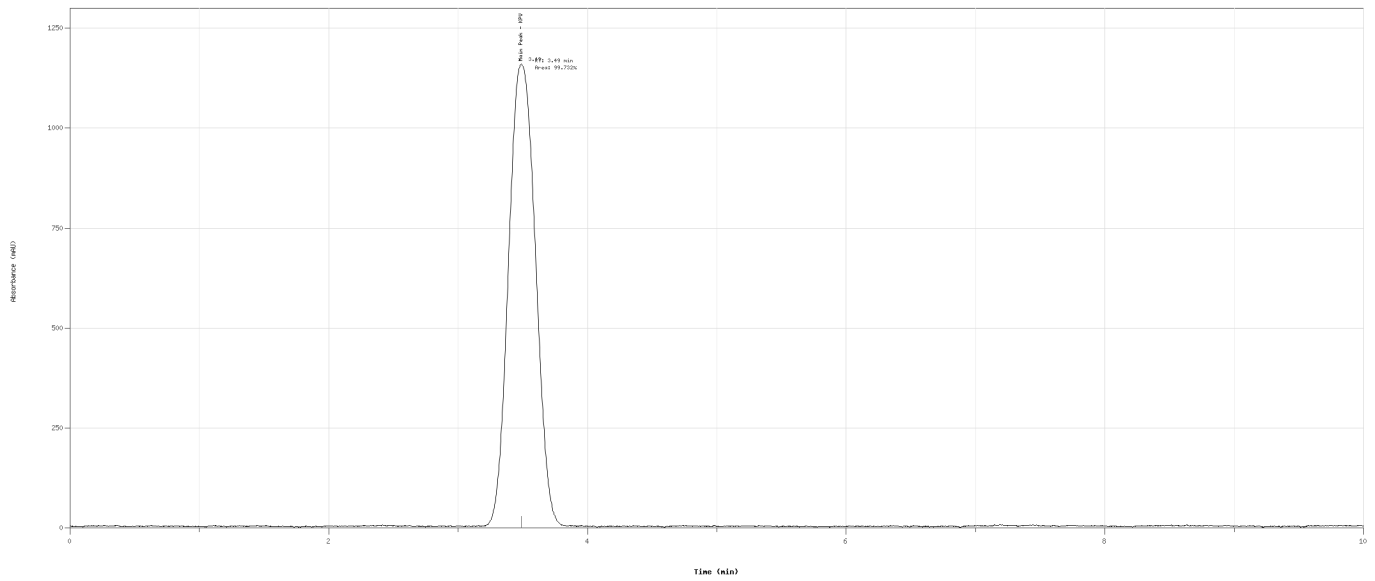

METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	96%	4%
2min	96%	4%
10min	12%	88%
12min	12%	88%

TECHNICAL NOTE

Gradient RP-HPLC-UV screening method with UV detection at 220 nm. Runtime 12.0 min.


COMMENTS

Chromatographic analysis confirms a consistent and reliable purity profile across the sample.

LC-MS MASS SPECTRUM

Sample: KPV
Report ID: 078-2025-004877
Reference MW: 402.50 Da
Ionization: ESI+

Acquisition: LC-MS
Profile: HESI-Orbitrap

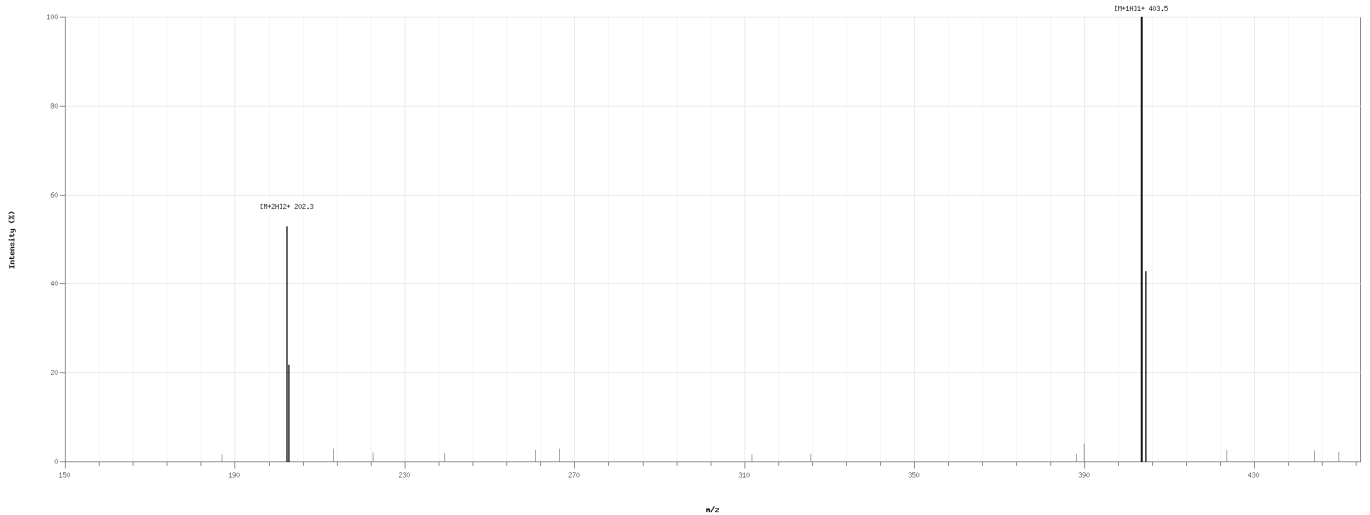

Charge-state distribution and isotope clustering consistent with the analyzed sample.

ANALYSIS & METHODOLOGY

STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

HPLC-UV: High-Performance Liquid Chromatography with Ultraviolet detection. Additional testing includes bioburden screening, endotoxin analysis and heavy metals assessment.

BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 1000
Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 100

ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
Bacterial Endotoxin USP <85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	< 0.001	EU/mg	> 0.5

HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
Arsenic Elemental Impurities Screening	Not detected	ppm	>= 1.5
Cadmium Elemental Impurities Screening	Not detected	ppm	>= 0.5
Cobalt Elemental Impurities Screening	Not detected	ppm	>= 25
Lead Elemental Impurities Screening	Not detected	ppm	>= 1.5

TEST	RESULT	UNIT	REPORTING LIMIT
Nickel Elemental Impurities Screening	Not detected	ppm	>= 25
Quicksilver Elemental Impurities Screening	Not detected	ppm	>= 1.5
Vanadium Elemental Impurities Screening	Not detected	ppm	>= 25

TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

COMPOUND REFERENCE

PARAMETER	KPV
PUBCHEM CID	90474670
CAS	2828433-34-5
MOLECULAR FORMULA	C18H34N4O6
MOLECULAR WEIGHT	402.5 g/mol

METHOD SPECIFICATION

PARAMETER	EARLY-ELUTING SHORT PEPTIDE RP-HPLC
ANALYTICAL MODE	Short peptide RP-HPLC-UV screening
COLUMN	C18 peptide column, short-gradient configuration
MOBILE PHASE A	Water + 0.1% TFA
MOBILE PHASE B	Acetonitrile + 0.1% TFA
FLOW RATE	1.0 mL/min
DETECTION	UV 220 nm
INJECTION VOLUME	10 uL
RUNTIME	10.0 min
SAMPLE DILUENT	Aqueous organic diluent compatible with RP-HPLC
SAMPLE PREPARATION	Direct dilution with clarification before analysis

INSTRUMENT PLATFORM

PARAMETER	STANDARD HPLC-UV PLATFORM
SYSTEM TYPE	Analytical HPLC system
DETECTOR	UV/VIS detector
ACQUISITION	Chromatographic acquisition and integration software
REVIEW MODE	Retention-time and response-profile review

PARAMETER	STANDARD HPLC-UV PLATFORM
WORKFLOW NOTE	Used for routine peptide purity and identity screening

ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
IDENTITY	Retention-time and profile agreement with reference expectations	Chromatographic identity review
PURITY	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
QUANTITY	Measured content reviewed against the declared sample strength	Report-level analytical summary
BIOBURDEN	Not detected or within stated reporting limits	Microbial screening table
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

Verification URL synaptica-labs.com/verify-report/

Report ID SYN-2026-004877

Verification Key VK-D2HH-FLLD

SCAN TO VERIFY



DIGITAL SIGNATURE



DIGITALLY SIGNED BY:

Martin Saar

Date: 2026.03.19

14:35:39 +02'00'

Director

info@synaptica-labs.com

Analysis date: Mar 18, 2026

Report generated: Mar 19, 2026

Analytical testing performed by Synaptica Analytics -
Analytical Services Division

Synaptica Analytics
SYN-2026-004877
Laboratory Analysis Report
VK-D2HH-FLLD

VERIFY AT
synaptica-labs.com/verify-report/