

## Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE <b>CJC-1295 No DAC</b>	RECEIVED DATE <b>Mar 31, 2026</b>	ANALYSIS DATE <b>Apr 06, 2026</b>	REPORT GENERATED <b>Apr 07, 2026</b>
STRENGTH	<b>10mg</b>	MANUFACTURER	<b>PepticoresAminos</b>
BATCH NUMBER	<b>PC-CJ10-0103T</b>	LAB CODE	<b>982-1</b>
CLIENT	<b>www.pepticoresAminos.net</b>		

## SAMPLE INFORMATION

**CJC-1295 No DAC****10MG**FORM **White powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-CJ10-0103T**CAP / CRIMP COLOR **trasp. yellow/silver**RECEIVED DATE **Mar 31, 2026**

SAMPLE IMAGE


## ANALYTICAL SUMMARY

IDENTITY	<b>CJC-1295 (mod GRF 1-29)</b>
PURITY	<b>99.791%</b>
QUANTITY	<b>11.82mg</b>
BATCH	<b>PC-CJ10-0103T</b>
MANUFACTURER	<b>PepticoresAminos</b>

# RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm

Sample ID: CJC-1235 No DIC  
Report ID: 2019-2020-04007  
Method: RP-HPLC-UV Method For Peptide Analysis  
Detector: UV 220 nm | Runtime: 12.0 min

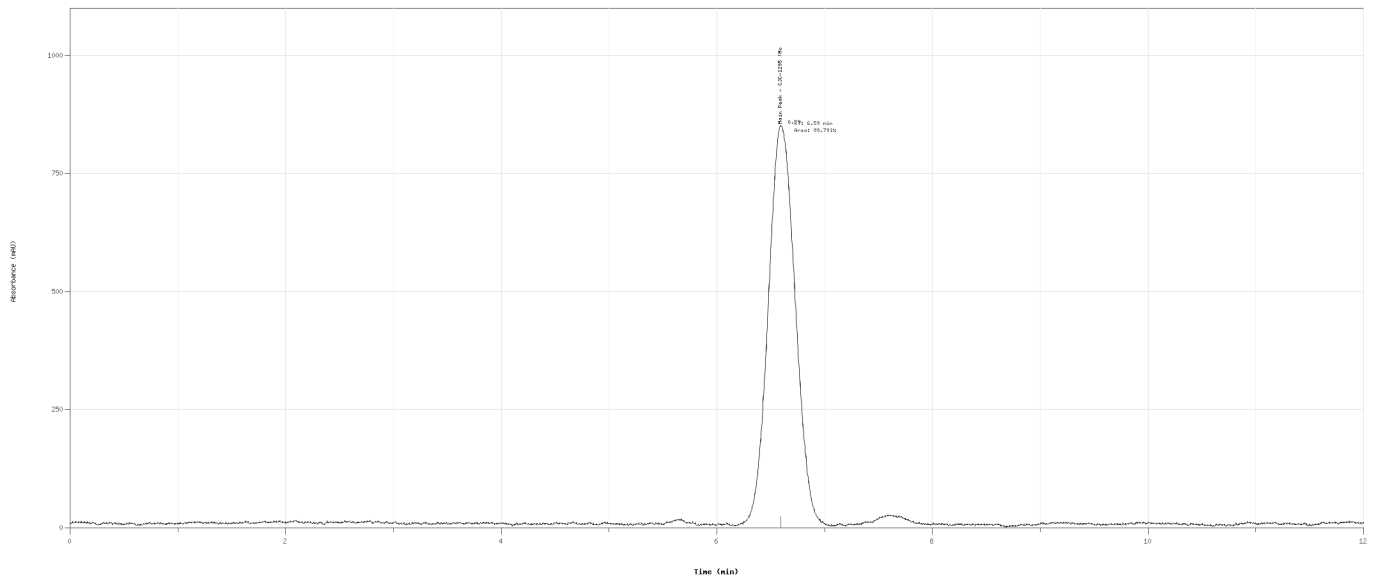

## METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	92%	8%
2min	92%	8%
10min	10%	90%
12min	10%	90%

## TECHNICAL NOTE

Gradient RP-HPLC-UV screening method with UV detection at 220 nm. Runtime 12.0 min.


## COMMENTS

The sample demonstrates conformity with expected analytical parameters and acceptable impurity levels.

## LC-MS MASS SPECTRUM

Sample: CJC-1295 (Prod GSP 1-29)  
 Report ID: 219-2024-04887  
 Reference MW: 3367.9 Da  
 Ionization: ESI+

Acquisition: LC-MS  
 Profile: Holes - Centroid

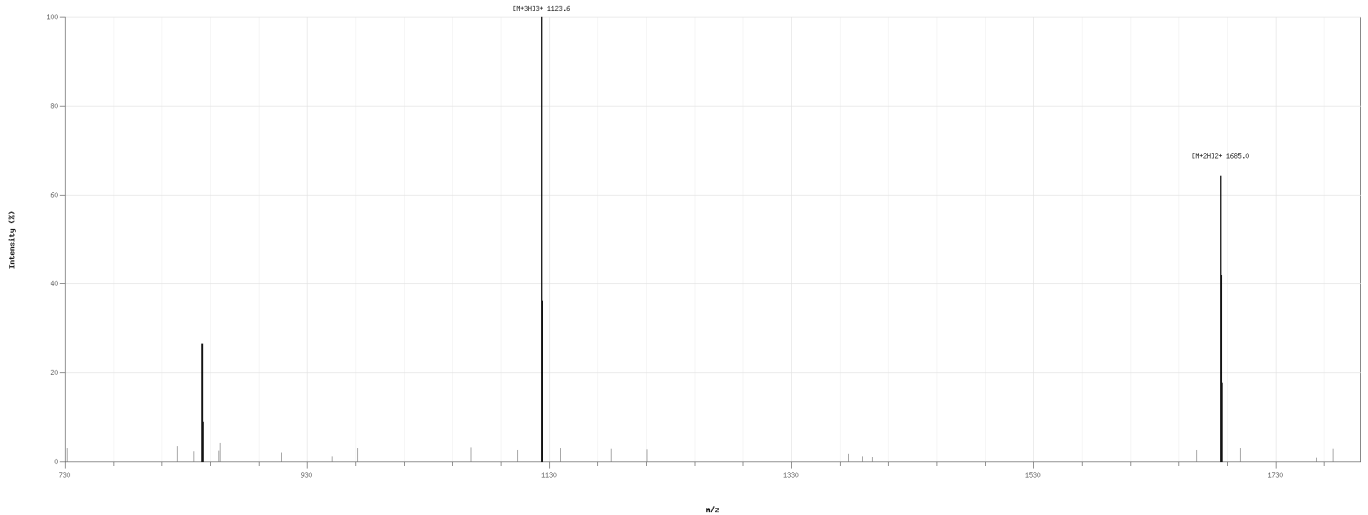

Charge-state distribution and isotope clustering consistent with the analyzed sample.

## ANALYSIS & METHODOLOGY

### STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

HPLC-UV: High-Performance Liquid Chromatography with Ultraviolet detection. Additional testing includes bioburden screening, endotoxin analysis and heavy metals assessment.

### BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Total Aerobic Microbial Count</b> USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 1000
<b>Total Yeast and Mold Count</b> USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 100

### ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Bacterial Endotoxin</b> USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	< 0.001	EU/mg	> 0.5

### HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Arsenic</b> Elemental Impurities Screening	Not detected	ppm	>= 1.5
<b>Cadmium</b> Elemental Impurities Screening	Not detected	ppm	>= 0.5
<b>Cobalt</b> Elemental Impurities Screening	Not detected	ppm	>= 25
<b>Lead</b> Elemental Impurities Screening	Not detected	ppm	>= 1.5

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Nickel</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>
<b>Quicksilver</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 1.5</b>
<b>Vanadium</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>

## TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

### METHOD SPECIFICATION

PARAMETER	RP-HPLC-UV METHOD FOR PEPTIDE ANALYSIS
<b>ANALYTICAL MODE</b>	Purity assessment of peptide sample by RP-HPLC-UV
<b>COLUMN</b>	C18 peptide column, 150 x 4.6 mm equivalent
<b>MOBILE PHASE A</b>	Water + 0.1% TFA
<b>MOBILE PHASE B</b>	Acetonitrile + 0.1% TFA
<b>FLOW RATE</b>	0.8 mL/min
<b>DETECTION</b>	UV 220 nm
<b>INJECTION VOLUME</b>	10 uL
<b>RUNTIME</b>	12.0 min
<b>SAMPLE DILUENT</b>	Aqueous organic diluent compatible with peptide analysis
<b>SAMPLE PREPARATION</b>	Diluted, mixed and clarified before injection

### INSTRUMENT PLATFORM

PARAMETER	STANDARD HPLC-UV PLATFORM
<b>SYSTEM TYPE</b>	Analytical HPLC system
<b>DETECTOR</b>	UV/VIS detector
<b>ACQUISITION</b>	Chromatographic acquisition and integration software
<b>REVIEW MODE</b>	Retention-time and response-profile review
<b>WORKFLOW NOTE</b>	Used for routine peptide purity and identity screening

### ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
<b>IDENTITY</b>	Retention-time and profile agreement with reference expectations	Chromatographic identity review
<b>PURITY</b>	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
<b>QUANTITY</b>	Measured content reviewed against the declared sample strength	Report-level analytical summary
<b>BIOBURDEN</b>	Not detected or within stated reporting limits	Microbial screening table

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

## VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

**Verification URL** [synaptica-labs.com/verify-report/](https://synaptica-labs.com/verify-report/)

**Report ID** SYN-2026-004887

**Verification Key** VK-Y6Z7-8ZDX

SCAN TO VERIFY



## DIGITAL SIGNATURE



**DIGITALLY SIGNED BY:**

**Martin Saar**

Date: 2026.04.07

15:23:47 +02'00'

Director

[info@synaptica-labs.com](mailto:info@synaptica-labs.com)

Analysis date: Apr 06, 2026

Report generated: Apr 07, 2026

Analytical testing performed by Synaptica Analytics -

Analytical Services Division

Synaptica Analytics  
**SYN-2026-004887**  
Laboratory Analysis Report  
**VK-Y6Z7-8ZDX**

**VERIFY AT**  
[synaptica-labs.com/verify-report/](https://synaptica-labs.com/verify-report/)