

Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE SS-31	RECEIVED DATE May 06, 2026	ANALYSIS DATE May 12, 2026	REPORT GENERATED May 13, 2026
STRENGTH	30mg	MANUFACTURER	PeptiCoreAminos
BATCH NUMBER	PC-SS30-0428L	LAB CODE	987-1
CLIENT	www.peptiCoreAminos.net		

SAMPLE INFORMATION

SS-31**30MG**FORM **White powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-SS30-0428L**CAP / CRIMP COLOR **White/Silver**RECEIVED DATE **May 06, 2026**

SAMPLE IMAGE


ANALYTICAL SUMMARY

IDENTITY	SS-31
PURITY	99.972%
QUANTITY	31.76mg
BATCH	PC-SS30-0428L
MANUFACTURER	PeptiCoreAminos

RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm | Runtime: 12.0 min

Sample ID: SS-01
Report ID: 2024-02-05-094007
Method: RP-HPLC-UV Method For Peptide Analysis
Detector: UV 220 nm | Runtime: 12.0 min

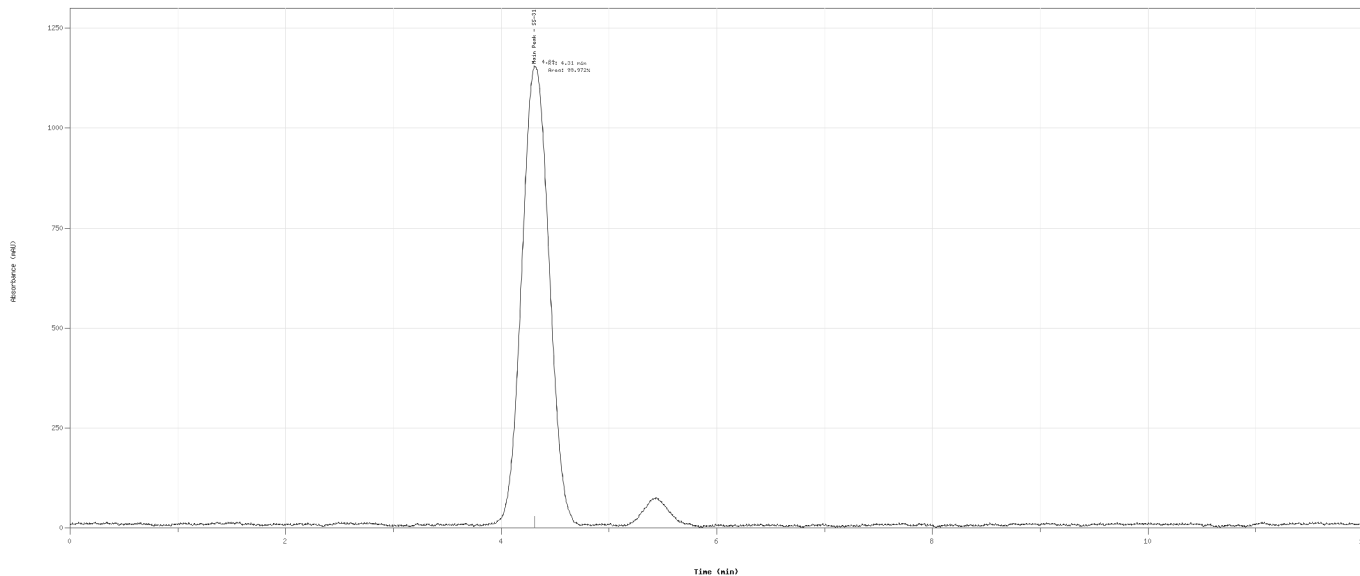

METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	92%	8%
2min	92%	8%
10min	10%	90%
12min	10%	90%

TECHNICAL NOTE

Results reported herein apply exclusively to the sample received and analyzed by the laboratory. Total runtime: 12.0 minutes.


COMMENTS

The evaluated material meets the defined analytical specifications for identity, purity and impurity profile based on the applied RP-HPLC-UV method.

LC-MS MASS SPECTRUM

Sample: 22-24
 Report ID: 224-2025-04907
 Reference MW: 639.80 Da
 Ionization: ESI+

Acquisition: LC-MS
 Profile: Total Ion Chromatogram

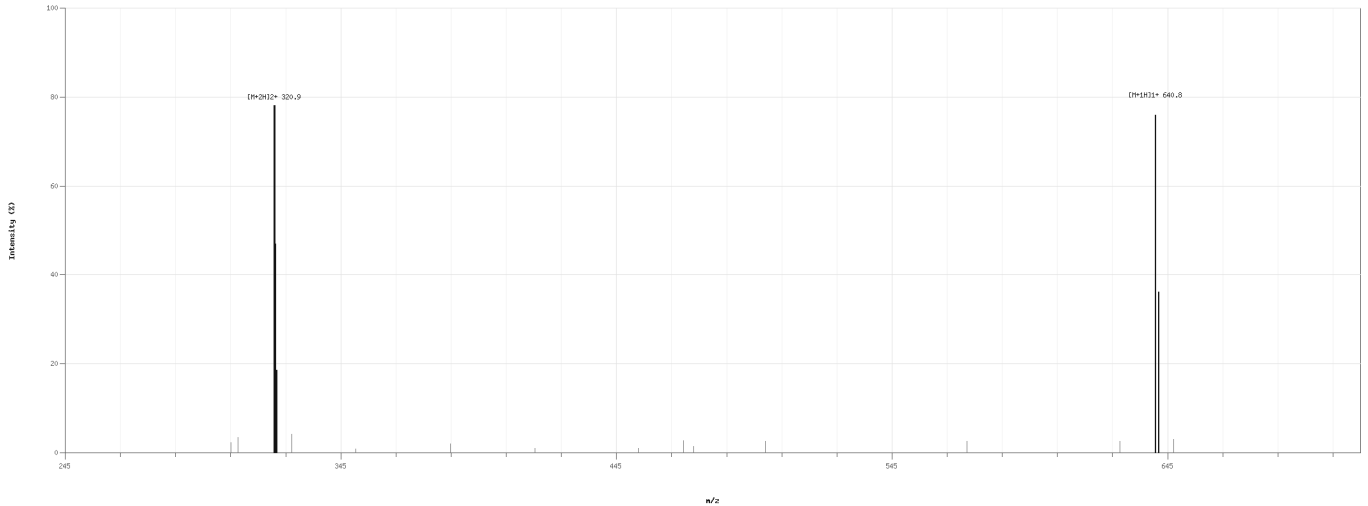

Observed ion distribution is consistent with the expected mass profile of the submitted analyte.

ANALYSIS & METHODOLOGY

STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

RP-HPLC-UV analysis was conducted under standardized conditions. Retention time, peak symmetry and analytical response were reviewed against established internal benchmarks.

BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 1000
Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 100

ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
Bacterial Endotoxin USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	< 0.001	EU/mg	> 0.5

HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
Arsenic Elemental Impurities Screening	Not detected	ppm	>= 1.5
Cadmium Elemental Impurities Screening	Not detected	ppm	>= 0.5
Cobalt Elemental Impurities Screening	Not detected	ppm	>= 25
Lead Elemental Impurities Screening	Not detected	ppm	>= 1.5

TEST	RESULT	UNIT	REPORTING LIMIT
Nickel Elemental Impurities Screening	Not detected	ppm	>= 25
Quicksilver Elemental Impurities Screening	Not detected	ppm	>= 1.5
Vanadium Elemental Impurities Screening	Not detected	ppm	>= 25

TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

COMPOUND REFERENCE

PARAMETER	SS-31
PUBCHEM CID	11764719
MOLECULAR FORMULA	C32H49N9O5
MOLECULAR WEIGHT	639.8 g/mol

METHOD SPECIFICATION

PARAMETER	RP-HPLC-UV METHOD FOR PEPTIDE ANALYSIS
ANALYTICAL MODE	Purity assessment of peptide sample by RP-HPLC-UV
COLUMN	C18 peptide column, 150 x 4.6 mm equivalent
MOBILE PHASE A	Water + 0.1% TFA
MOBILE PHASE B	Acetonitrile + 0.1% TFA
FLOW RATE	0.8 mL/min
DETECTION	UV 220 nm
INJECTION VOLUME	10 uL
RUNTIME	12.0 min
SAMPLE DILUENT	Aqueous organic diluent compatible with peptide analysis
SAMPLE PREPARATION	Diluted, mixed and clarified before injection

INSTRUMENT PLATFORM

PARAMETER	STANDARD HPLC-UV PLATFORM
SYSTEM TYPE	Analytical HPLC system
DETECTOR	UV/VIS detector
ACQUISITION	Chromatographic acquisition and integration software
REVIEW MODE	Retention-time and response-profile review
WORKFLOW NOTE	Used for routine peptide purity and identity screening

ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
IDENTITY	Retention-time and profile agreement with reference expectations	Chromatographic identity review
PURITY	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
QUANTITY	Measured content reviewed against the declared sample strength	Report-level analytical summary
BIOBURDEN	Not detected or within stated reporting limits	Microbial screening table
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

Verification URL synaptica-labs.com/verify-report

Report ID SYN-2026-004907

Verification Key VK-UZ79-H29D

SCAN TO VERIFY



DIGITAL SIGNATURE



DIGITALLY SIGNED BY:
Martin Saar
Date: 2026.05.13
17:06:21 +02'00'
Director

info@synaptica-labs.com

Analysis date: May 12, 2026

Report generated: May 13, 2026

Analytical testing performed by Synaptica Analytics -
Analytical Services Division

Synaptica Analytics
SYN-2026-004907
Laboratory Analysis Report
VK-UZ79-H29D

VERIFY AT
synaptica-labs.com/verify-report