

Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

| | | | |
|------------------------------|--------------------------------------|--------------------------------------|---|
| SAMPLE Tesamorelin | RECEIVED DATE May 18, 2026 | ANALYSIS DATE May 22, 2026 | REPORT GENERATED May 26, 2026 |
| STRENGTH | 10mg | MANUFACTURER | PepticoAminos |
| BATCH NUMBER | PC-TS10-0427L | LAB CODE | 887-2 |
| CLIENT | www.pepticoaminos.net | | |

SAMPLE INFORMATION

Tesamorelin

10MG**FORM** White powder in a glass vial**SAMPLE SUBMISSION** Sample provided by customer**BATCH** PC-TS10-0427L**CAP / CRIMP COLOR** trasp.blue/silver**RECEIVED DATE** May 18, 2026

SAMPLE IMAGE


ANALYTICAL SUMMARY

| | |
|---------------------|---------------|
| IDENTITY | Tesamorelin |
| PURITY | 99.563% |
| QUANTITY | 10.54mg |
| BATCH | PC-TS10-0427L |
| MANUFACTURER | PepticoAminos |

RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm | Runtime: 14.0 min

Sample ID: Tesamorelin
Report ID: 2024-02-01-000009
Method: RP-HPLC-UV Long Peptide
Detector: UV 220 nm | Runtime: 14.0 min

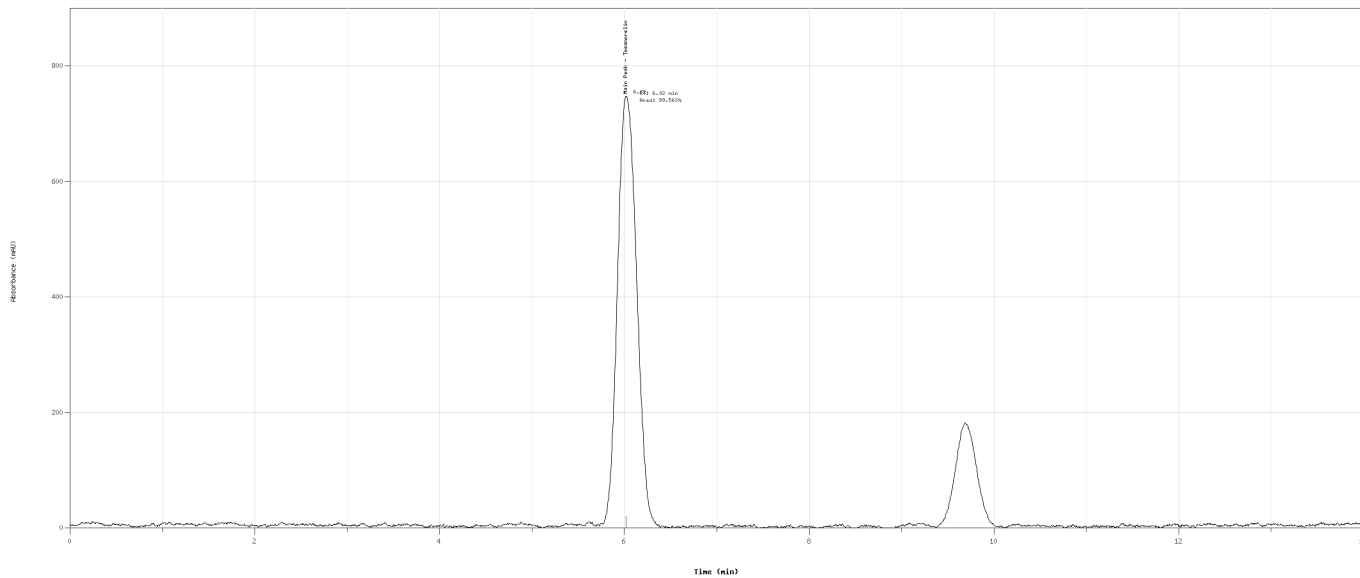

METHOD

| TIME | H2O + 0.1% TFA | ACN + 0.1% TFA |
|-------|----------------|----------------|
| 0min | 90% | 10% |
| 2min | 90% | 10% |
| 10min | 8% | 92% |
| 12min | 8% | 92% |
| 14min | 8% | 92% |

TECHNICAL NOTE

Analysis performed by RP-HPLC-UV at 220 nm using a gradient elution program. Total runtime: 14.0 minutes.


COMMENTS

The sample complies with the defined analytical specifications for identity, purity and impurity profile under the applied RP-HPLC-UV method.

LC-MS MASS SPECTRUM

Sample: Testosterone
 Report ID: 2024-03-01-04255
 Reference MS: 5136.0 Da
 Ionization: ESI+

Acquisition: LC-MS
 Profile: Testosterone

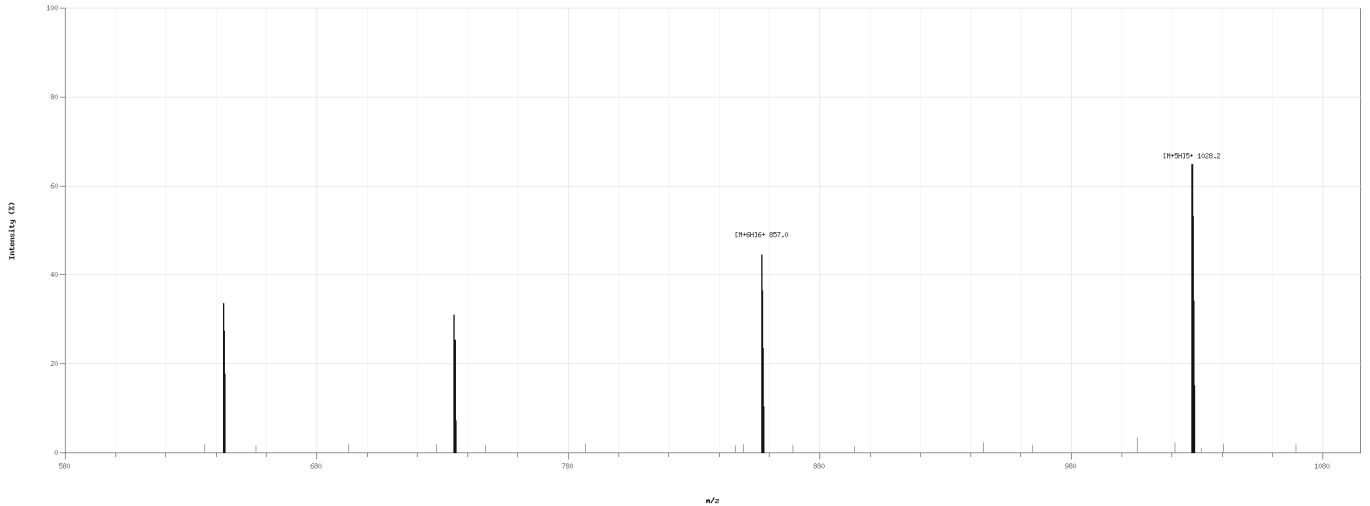

The recorded mass spectrum shows signals compatible with the expected molecular profile of the sample.

ANALYSIS & METHODOLOGY

STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

Sample analyzed by reverse-phase HPLC with UV detection using controlled analytical parameters. Chromatographic behavior and purity response were assessed through internal laboratory criteria.

BIOBURDEN

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|--------------|-------|-----------------|
| Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method | Not detected | CFU/g | >= 1000 |
| Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method | Not detected | CFU/g | >= 100 |

ENDOTOXIN ANALYSIS

| TEST | RESULT | UNIT | REPORTING LIMIT |
|---|---------|-------|-----------------|
| Bacterial Endotoxin USP <85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test | < 0.001 | EU/mg | > 0.5 |

HEAVY METALS

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|--------------|------|-----------------|
| Arsenic Elemental Impurities Screening | Not detected | ppm | >= 1.5 |
| Cadmium Elemental Impurities Screening | Not detected | ppm | >= 0.5 |
| Cobalt Elemental Impurities Screening | Not detected | ppm | >= 25 |
| Lead Elemental Impurities Screening | Not detected | ppm | >= 1.5 |

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|---------------------|------------|------------------|
| Nickel Elemental Impurities Screening | Not detected | ppm | >= 25 |
| Quicksilver Elemental Impurities Screening | Not detected | ppm | >= 1.5 |
| Vanadium Elemental Impurities Screening | Not detected | ppm | >= 25 |

TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

COMPOUND REFERENCE

| PARAMETER | TESAMORELIN |
|--------------------------|-----------------|
| PUBCHEM CID | 16137828 |
| CAS | 218949-48-5 |
| MOLECULAR FORMULA | C221H366N72O67S |
| MOLECULAR WEIGHT | 5136.0 g/mol |

METHOD SPECIFICATION

| PARAMETER | LONG PEPTIDE EXTENDED RP-HPLC-UV METHOD |
|---------------------------|--|
| ANALYTICAL MODE | Extended gradient RP-HPLC-UV peptide purity screen |
| COLUMN | C18 peptide column, extended-gradient configuration |
| MOBILE PHASE A | Water + 0.1% TFA |
| MOBILE PHASE B | Acetonitrile + 0.1% TFA |
| FLOW RATE | 0.7 mL/min |
| DETECTION | UV 220 nm |
| INJECTION VOLUME | 10 uL |
| RUNTIME | 14.0 min |
| SAMPLE DILUENT | Water/acetonitrile compatible diluent |
| SAMPLE PREPARATION | Diluted to method range and clarified before injection |

INSTRUMENT PLATFORM

| PARAMETER | HIGH-RESOLUTION UPLC/HPLC-UV PLATFORM |
|--------------------|--|
| SYSTEM TYPE | High-resolution LC platform |
| DETECTOR | UV/VIS detector |
| ACQUISITION | Chromatographic acquisition and integration software |
| REVIEW MODE | Gradient profile review with peak integration |

| PARAMETER | HIGH-RESOLUTION UPLC/HPLC-UV PLATFORM |
|---------------|--|
| WORKFLOW NOTE | Used for long peptide and multi-component profile review |

ANALYTICAL CRITERIA

| PARAMETER | ACCEPTANCE FRAMEWORK | BASIS |
|--------------|---|--------------------------------------|
| IDENTITY | Retention-time and profile agreement with reference expectations | Chromatographic identity review |
| PURITY | NLT 98.0% unless a stricter report-specific specification is declared | Integrated RP-HPLC-UV purity profile |
| QUANTITY | Measured content reviewed against the declared sample strength | Report-level analytical summary |
| BIOBURDEN | Not detected or within stated reporting limits | Microbial screening table |
| ENDOTOXIN | Below stated reporting limit / internal screening threshold | Endotoxin analysis table |
| HEAVY METALS | Below individual reporting limits where screened | Elemental impurities screening table |

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

Verification URL synaptica-labs.com/verify-report

Report ID SYN-2026-004939

Verification Key VK-RY8P-G9D2

SCAN TO VERIFY



DIGITAL SIGNATURE



DIGITALLY SIGNED BY:

Martin Saar

Date: 2026.05.26

10:52:32 +02'00'

Director

info@synaptica-labs.com

Analysis date: May 22, 2026

Report generated: May 26, 2026

Analytical testing performed by Synaptica Analytics -

Analytical Services Division

Synaptica Analytics
SYN-2026-004939
Laboratory Analysis Report
VK-RY8P-G9D2

VERIFY AT
synaptica-labs.com/verify-report