

Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

| | | | |
|--------------------------|--------------------------------------|--------------------------------------|---|
| SAMPLE BPC-157 | RECEIVED DATE May 18, 2026 | ANALYSIS DATE May 22, 2026 | REPORT GENERATED May 25, 2026 |
| STRENGTH | 10mg | MANUFACTURER | PepticoresAminos |
| BATCH NUMBER | PC-BP10-0526E | LAB CODE | 673-1 |
| CLIENT | www.pepticoresaminos.us | | |

SAMPLE INFORMATION

BPC-157**10MG**FORM **White lyophilized powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-BP10-0526E**CAP / CRIMP COLOR **Clear yellow/silver**RECEIVED DATE **May 18, 2026**

SAMPLE IMAGE


ANALYTICAL SUMMARY

| | |
|--------------|-------------------------|
| IDENTITY | BPC-157 |
| PURITY | 99.934% |
| QUANTITY | 13.43mg |
| BATCH | PC-BP10-0526E |
| MANUFACTURER | PepticoresAminos |

RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm | Runtime: 12.0 min

Sample ID: BPC-157
Report ID: 2024-02-01-00003
Method: RP-HPLC-UV Method For Peptide Analysis
Detector: UV 220 nm | Runtime: 12.0 min

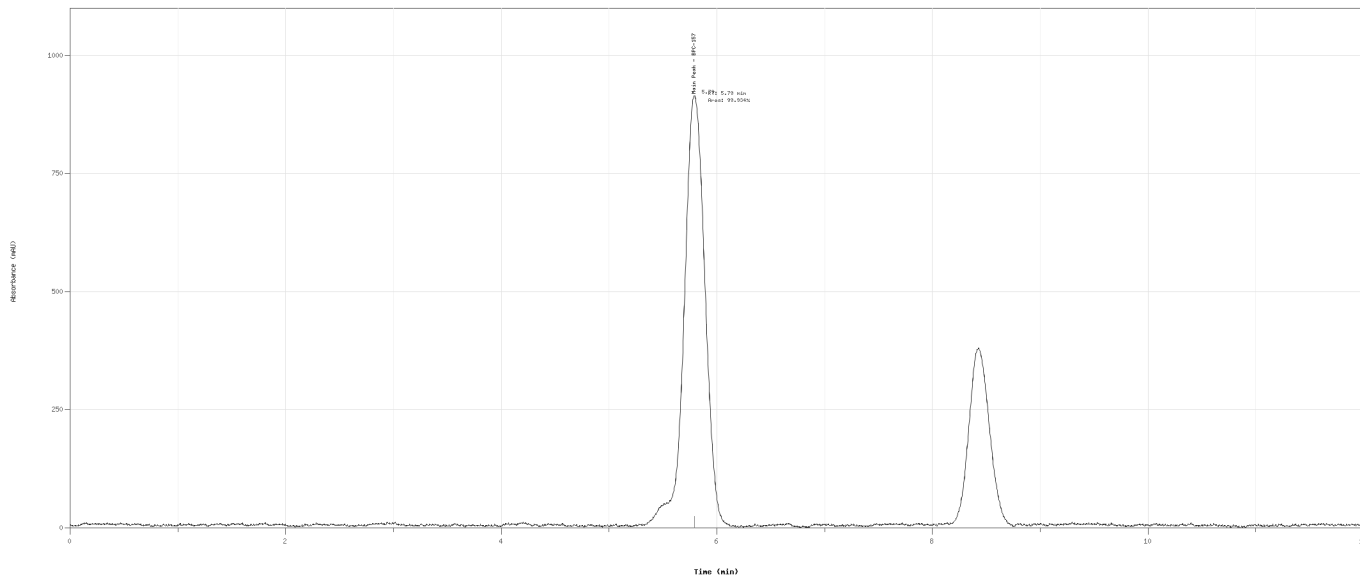

METHOD

| TIME | H2O + 0.1% TFA | ACN + 0.1% TFA |
|-------|----------------|----------------|
| 0min | 95% | 5% |
| 2min | 95% | 5% |
| 10min | 8% | 92% |
| 12min | 8% | 92% |

TECHNICAL NOTE

This report reflects the analytical findings obtained for the submitted sample under the stated test conditions. Total runtime: 12.0 minutes.


COMMENTS

The sample complies with the defined analytical specifications for identity, purity and impurity profile under the applied RP-HPLC-UV method.

LC-MS MASS SPECTRUM

Sample: BPC-187
 Report ID: 2024-2025-044953
 Reference MW: 1419.5 Da
 Ionization: ESI+

Acquisition: LC-MS
 Profile: Total Ion Chromatogram

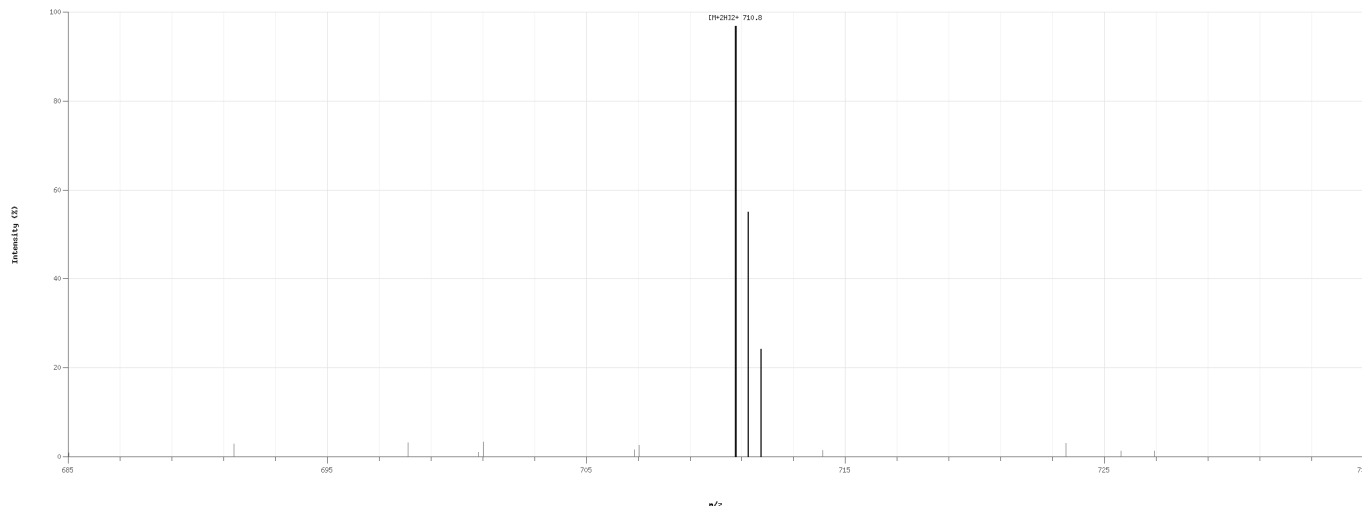

Charge-state distribution and isotope clustering are consistent with the expected analytical mass response.

ANALYSIS & METHODOLOGY

STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

RP-HPLC-UV analysis was conducted under standardized conditions. Retention time, peak symmetry and analytical response were reviewed against established internal benchmarks.

BIOBURDEN

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|--------------|-------|-----------------|
| Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method | Not detected | CFU/g | >= 1000 |
| Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method | Not detected | CFU/g | >= 100 |

ENDOTOXIN ANALYSIS

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|---------|-------|-----------------|
| Bacterial Endotoxin USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test | < 0.001 | EU/mg | > 0.5 |

HEAVY METALS

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|--------------|------|-----------------|
| Arsenic Elemental Impurities Screening | Not detected | ppm | >= 1.5 |
| Cadmium Elemental Impurities Screening | Not detected | ppm | >= 0.5 |
| Cobalt Elemental Impurities Screening | Not detected | ppm | >= 25 |
| Lead Elemental Impurities Screening | Not detected | ppm | >= 1.5 |

| TEST | RESULT | UNIT | REPORTING LIMIT |
|--|---------------------|------------|------------------|
| Nickel Elemental Impurities Screening | Not detected | ppm | >= 25 |
| Quicksilver Elemental Impurities Screening | Not detected | ppm | >= 1.5 |
| Vanadium Elemental Impurities Screening | Not detected | ppm | >= 25 |

TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

COMPOUND REFERENCE

| PARAMETER | BPC-157 |
|--------------------------|--------------|
| PUBCHEM CID | 9941957 |
| CAS | 137525-51-0 |
| MOLECULAR FORMULA | C62H98N16O22 |
| MOLECULAR WEIGHT | 1419.5 g/mol |

METHOD SPECIFICATION

| PARAMETER | RP-HPLC-UV METHOD FOR PEPTIDE ANALYSIS |
|---------------------------|---|
| ANALYTICAL MODE | Purity assessment of peptide sample by RP-HPLC-UV |
| COLUMN | C18 peptide column, 150 x 4.6 mm equivalent |
| MOBILE PHASE A | Water + 0.1% TFA |
| MOBILE PHASE B | Acetonitrile + 0.1% TFA |
| FLOW RATE | 1.0 mL/min |
| DETECTION | UV 220 nm |
| INJECTION VOLUME | 10 uL |
| RUNTIME | 12.0 min |
| SAMPLE DILUENT | Water/acetonitrile compatible diluent |
| SAMPLE PREPARATION | Diluted to working concentration and filtered/clarified |

INSTRUMENT PLATFORM

| PARAMETER | STANDARD HPLC-UV PLATFORM |
|--------------------|--|
| SYSTEM TYPE | Analytical HPLC system |
| DETECTOR | UV/VIS detector |
| ACQUISITION | Chromatographic acquisition and integration software |
| REVIEW MODE | Retention-time and response-profile review |

| PARAMETER | STANDARD HPLC-UV PLATFORM |
|---------------|--|
| WORKFLOW NOTE | Used for routine peptide purity and identity screening |

ANALYTICAL CRITERIA

| PARAMETER | ACCEPTANCE FRAMEWORK | BASIS |
|--------------|---|--------------------------------------|
| IDENTITY | Retention-time and profile agreement with reference expectations | Chromatographic identity review |
| PURITY | NLT 98.0% unless a stricter report-specific specification is declared | Integrated RP-HPLC-UV purity profile |
| QUANTITY | Measured content reviewed against the declared sample strength | Report-level analytical summary |
| BIOBURDEN | Not detected or within stated reporting limits | Microbial screening table |
| ENDOTOXIN | Below stated reporting limit / internal screening threshold | Endotoxin analysis table |
| HEAVY METALS | Below individual reporting limits where screened | Elemental impurities screening table |

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

Verification URL synaptica-labs.com/verify-report

Report ID SYN-2026-004953

Verification Key VK-GX9N-SFGV

SCAN TO VERIFY



DIGITAL SIGNATURE



DIGITALLY SIGNED BY:

Martin Saar

Date: 2026.05.25

13:53:48 +02'00'

Director

info@synaptica-labs.com

Analysis date: May 22, 2026

Report generated: May 25, 2026

Analytical testing performed by Synaptica Analytics -

Analytical Services Division

Synaptica Analytics
SYN-2026-004953
Laboratory Analysis Report
VK-GX9N-SFGV

VERIFY AT
synaptica-labs.com/verify-report