

## Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE <b>Epithalon</b>	RECEIVED DATE <b>May 28, 2026</b>	ANALYSIS DATE <b>Jun 01, 2026</b>	REPORT GENERATED <b>Jun 03, 2026</b>
STRENGTH	<b>10mg</b>	MANUFACTURER	<b>PepticoresAminos</b>
BATCH NUMBER	<b>PC-EP10-0510A</b>	LAB CODE	<b>982-3</b>
CLIENT	<b>www.pepticoresaminos.net</b>		

## SAMPLE INFORMATION

# Epithalon

**10MG**FORM **White powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-EP10-0510A**CAP / CRIMP COLOR **Clear/silver**RECEIVED DATE **May 28, 2026**

SAMPLE IMAGE


## ANALYTICAL SUMMARY

IDENTITY	<b>Epithalon</b>
PURITY	<b>99.920%</b>
QUANTITY	<b>10.06mg</b>
BATCH	<b>PC-EP10-0510A</b>
MANUFACTURER	<b>PepticoresAminos</b>

# RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm | Runtime: 12.0 min

Sample ID: Epithalon  
Report ID: 2024-0220-000007  
Method: RP-HPLC-UV General  
Detector: UV 220 nm | Runtime: 12.0 min

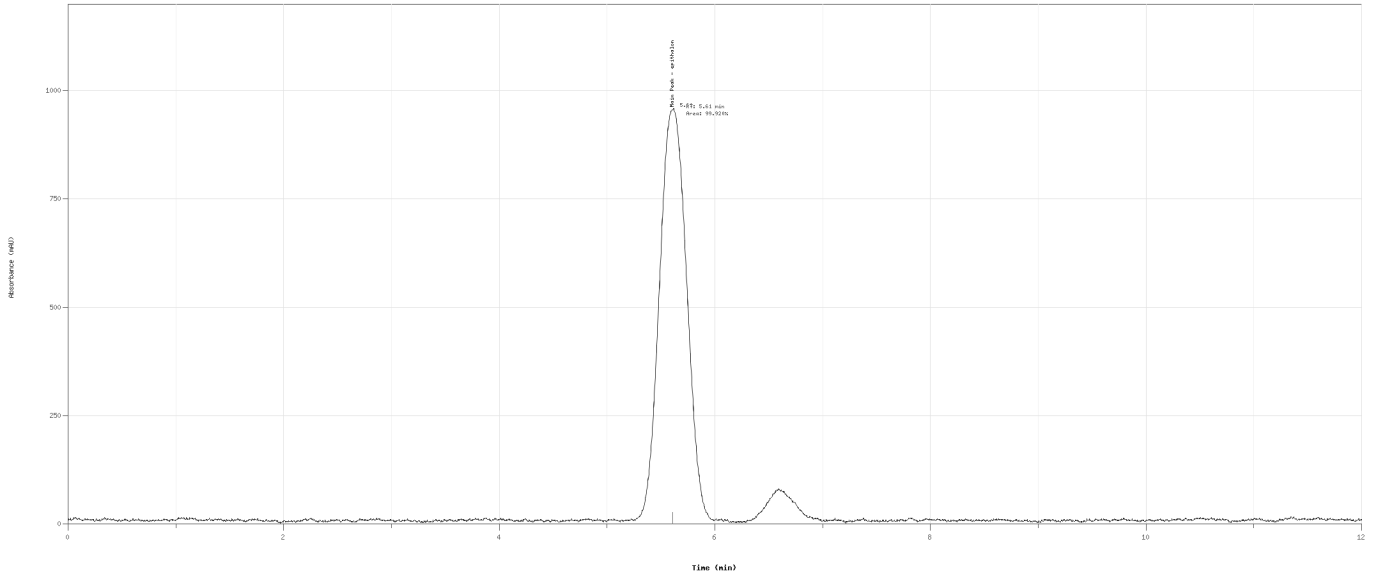

## METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	95%	5%
2min	95%	5%
10min	5%	95%
12min	5%	95%

## TECHNICAL NOTE

Results reported herein apply exclusively to the sample received and analyzed by the laboratory. Total runtime: 12.0 minutes.

## COMMENTS

The chromatographic result supports that the sample meets the defined analytical specifications for identity, purity and impurity profile based on the applied RP-HPLC-UV method.

## ANALYSIS & METHODOLOGY

### STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

Analysis performed using RP-HPLC-UV under validated laboratory conditions. Peak profile, retention behavior and purity response were evaluated against internal reference standards.

## BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Total Aerobic Microbial Count</b> USP <61>/Eur. Ph. 2.6.12. Plate Count Method	<b>Not detected</b>	<b>CFU/g</b>	<b>&gt;= 1000</b>

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Total Yeast and Mold Count</b> USP <61>/Eur. Ph. 2.6.12. Plate Count Method	<b>Not detected</b>	<b>CFU/g</b>	<b>&gt;= 100</b>

## ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Bacterial Endotoxin</b> USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	<b>&lt; 0.001</b>	<b>EU/mg</b>	<b>&gt; 0.5</b>

## HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
<b>Arsenic</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 1.5</b>
<b>Cadmium</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 0.5</b>
<b>Cobalt</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>
<b>Lead</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 1.5</b>
<b>Nickel</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>
<b>Quicksilver</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 1.5</b>
<b>Vanadium</b> Elemental Impurities Screening	<b>Not detected</b>	<b>ppm</b>	<b>&gt;= 25</b>

## TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

## METHOD SPECIFICATION

PARAMETER	GENERAL RP-HPLC-UV SCREENING
<b>ANALYTICAL MODE</b>	Reversed-phase HPLC purity and identity screen
<b>COLUMN</b>	C18 reversed-phase analytical column
<b>MOBILE PHASE A</b>	Water + 0.1% TFA
<b>MOBILE PHASE B</b>	Acetonitrile + 0.1% TFA
<b>FLOW RATE</b>	1.0 mL/min
<b>DETECTION</b>	UV 220 nm
<b>INJECTION VOLUME</b>	10 uL
<b>RUNTIME</b>	12.0 min
<b>SAMPLE DILUENT</b>	Water/acetonitrile compatible diluent
<b>SAMPLE PREPARATION</b>	Diluted, mixed and clarified prior to injection

## INSTRUMENT PLATFORM

PARAMETER	STANDARD HPLC-UV PLATFORM
SYSTEM TYPE	Analytical HPLC system
DETECTOR	UV/VIS detector
ACQUISITION	Chromatographic acquisition and integration software
REVIEW MODE	Retention-time and response-profile review
WORKFLOW NOTE	Used for routine peptide purity and identity screening

## ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
IDENTITY	Retention-time and profile agreement with reference expectations	Chromatographic identity review
PURITY	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
QUANTITY	Measured content reviewed against the declared sample strength	Report-level analytical summary
BIOBURDEN	Not detected or within stated reporting limits	Microbial screening table
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

## VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

**Verification URL** [synaptica-labs.com/verify-report](https://synaptica-labs.com/verify-report)

**Report ID** SYN-2026-004967

**Verification Key** VK-LU8L-YC4W

SCAN TO VERIFY



## DIGITAL SIGNATURE



**DIGITALLY SIGNED BY:**

**Martin Saar**

Date: 2026.06.03

18:21:55 +02'00'

Director

[info@synaptica-labs.com](mailto:info@synaptica-labs.com)

Analysis date: Jun 01, 2026

Report generated: Jun 03, 2026

Analytical testing performed by Synaptica Analytics -  
Analytical Services Division

Synaptica Analytics  
**SYN-2026-004967**  
Laboratory Analysis Report  
**VK-LU8L-YC4W**

**VERIFY AT**  
[synaptica-labs.com/verify-report](https://synaptica-labs.com/verify-report)