

Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE GLOW	RECEIVED DATE May 01, 2026	ANALYSIS DATE May 05, 2026	REPORT GENERATED May 07, 2026
STRENGTH	70mg	MANUFACTURER	PeptiCoreAminos
BATCH NUMBER	PC-GL70-0425L	LAB CODE	983-1
CLIENT	www.peptiCoreAminos.net		

SAMPLE INFORMATION

GLOW**70MG**FORM **Blue lyophilized powder in a glass vial**SAMPLE SUBMISSION **Sample provided by customer**BATCH **PC-GL70-0425L**CAP / CRIMP COLOR **Yellow/black**RECEIVED DATE **May 01, 2026**

SAMPLE IMAGE

ANALYTICAL SUMMARY

IDENTITY	GLOW
PURITY	99.853%
QUANTITY	72mg
BATCH	PC-GL70-0425L
MANUFACTURER	PeptiCoreAminos


BLEND COMPOSITION

COMPONENT	MEASURED MASS
GHK-Cu	51.42mg
TB-500 (TB4)	10.34mg
BPC-157	10.24mg

RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm | Runtime: 12.0 min

Sample ID: G1ow Blend
Report ID: 2024-02-20-1449373
Method: RP-HPLC-UV Blend Screen
Detector: UV 220 nm | Runtime: 12.0 min

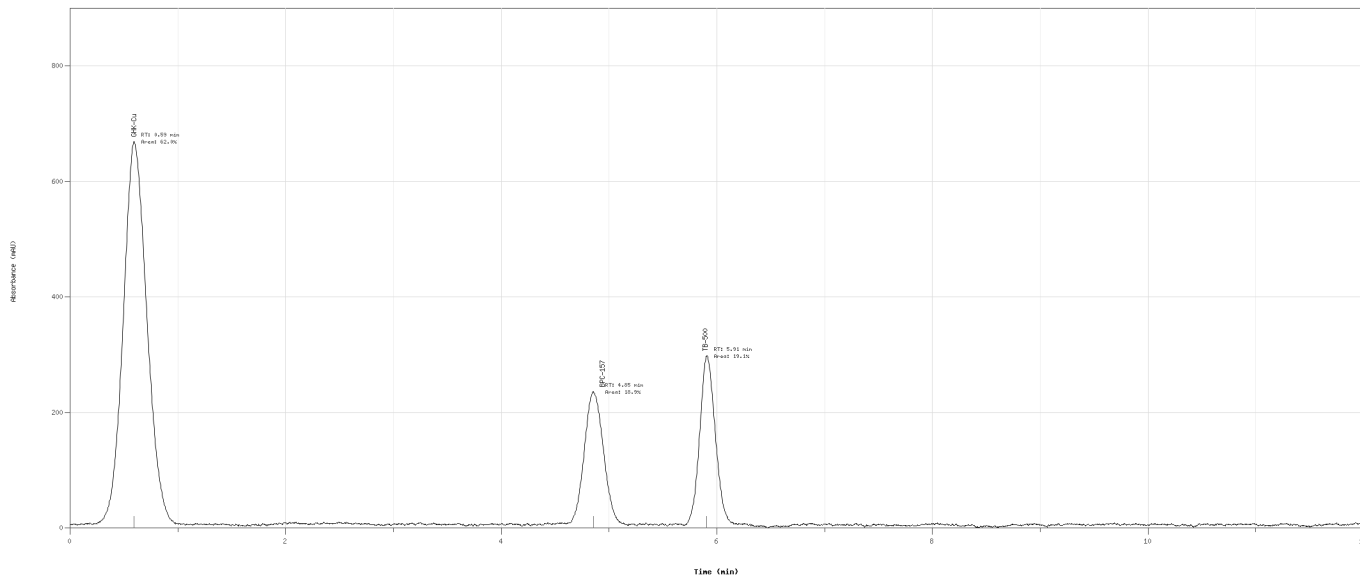

METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	95%	5%
2min	95%	5%
10min	12%	88%
12min	12%	88%

TECHNICAL NOTE

Analytical conclusions are limited to the tested blend and the conditions described in this report. Total runtime: 12.0 minutes.


COMMENTS

Analytical assessment indicates that the sample meets the defined specifications for identity, purity and impurity profile using the applied RP-HPLC-UV method.

LC-MS MASS SPECTRUM

Sample: 624e
Report ID: STN-2025-044973
Reference Basis: component-derived composite
Ionization: ESI+ Composite

Acquisition: LC-MS
Components: BPC-127, TBA, QM-Cu

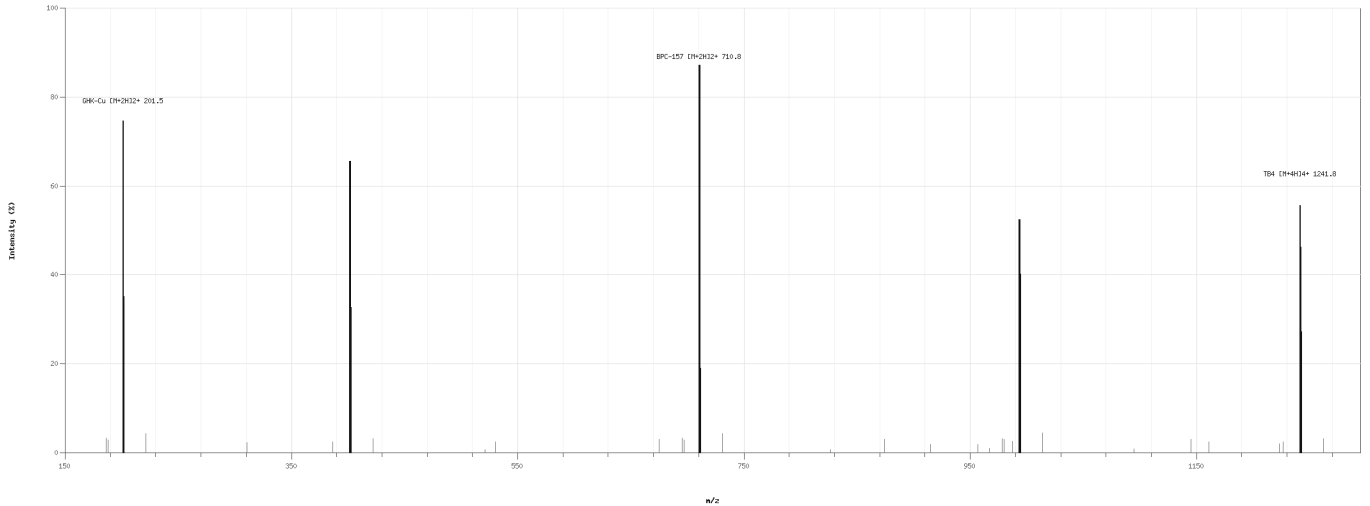

Charge-state distribution and clustered ion signals are consistent with the expected composite mass response of the sample.

ANALYSIS & METHODOLOGY

STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

Blend formulation analyzed by reverse-phase HPLC with UV detection under conditions suitable for multi-component separation. Component peak distribution and overall profile were assessed.

BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 1000
Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 100

ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
Bacterial Endotoxin USP <85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	< 0.001	EU/mg	> 0.5

HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
Arsenic Elemental Impurities Screening	Not detected	ppm	>= 1.5
Cadmium Elemental Impurities Screening	Not detected	ppm	>= 0.5
Cobalt Elemental Impurities Screening	Not detected	ppm	>= 25
Lead Elemental Impurities Screening	Not detected	ppm	>= 1.5

TEST	RESULT	UNIT	REPORTING LIMIT
Nickel Elemental Impurities Screening	Not detected	ppm	>= 25
Quicksilver Elemental Impurities Screening	Not detected	ppm	>= 1.5
Vanadium Elemental Impurities Screening	Not detected	ppm	>= 25

TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

BLEND COMPONENT REFERENCE

COMPONENT	PUBCHEM CID	CAS	MOLECULAR FORMULA	MOLECULAR WEIGHT
BPC-157	9941957	137525-51-0	C62H98N16O22	1419.5 g/mol
TB-500 (TB4)	45382195	77591-33-4	C212H350N56O78S	4963.0 g/mol
GHK-CU	139035031	49557-75-7	C14H21CuN6O4-	400.9 g/mol

METHOD SPECIFICATION

PARAMETER	MULTI-COMPONENT PEPTIDE BLEND RP-HPLC-UV METHOD
ANALYTICAL MODE	Multi-component RP-HPLC-UV peptide blend screen
COLUMN	C18 peptide column, multi-component gradient configuration
MOBILE PHASE A	Water + 0.1% TFA
MOBILE PHASE B	Acetonitrile + 0.1% TFA
FLOW RATE	0.8 mL/min
DETECTION	UV 220 nm
INJECTION VOLUME	10 uL
RUNTIME	12.0 min
SAMPLE DILUENT	Aqueous organic diluent compatible with peptide blends
SAMPLE PREPARATION	Diluted, mixed and clarified before component review

INSTRUMENT PLATFORM

PARAMETER	HIGH-RESOLUTION UPLC/HPLC-UV PLATFORM
SYSTEM TYPE	High-resolution LC platform
DETECTOR	UV/VIS detector
ACQUISITION	Chromatographic acquisition and integration software
REVIEW MODE	Gradient profile review with peak integration
WORKFLOW NOTE	Used for long peptide and multi-component profile review

ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
IDENTITY	Retention-time and profile agreement with reference expectations	Chromatographic identity review
PURITY	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
QUANTITY	Measured content reviewed against the declared sample strength	Report-level analytical summary
BIOBURDEN	Not detected or within stated reporting limits	Microbial screening table
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

Verification URL synaptica-labs.com/verify-report

Report ID SYN-2026-004973

Verification Key VK-WWWD-AHV8

SCAN TO VERIFY



DIGITAL SIGNATURE



DIGITALLY SIGNED BY:
Martin Saar
Date: 2026.05.07
17:55:04 +02'00'
Director

info@synaptica-labs.com

Analysis date: May 05, 2026

Report generated: May 07, 2026

Analytical testing performed by Synaptica Analytics -
Analytical Services Division

Synaptica Analytics
SYN-2026-004973
Laboratory Analysis Report
VK-WWWD-AHV8

VERIFY AT
synaptica-labs.com/verify-report