

Analysis Report

Official laboratory analysis summary for the submitted sample and associated quality-control review.

SAMPLE Tirzepatide	RECEIVED DATE May 13, 2026	ANALYSIS DATE May 18, 2026	REPORT GENERATED May 19, 2026
STRENGTH	10mg	MANUFACTURER	PepticoresAminos
BATCH NUMBER	PC-TZ10-2012B	LAB CODE	989-2
CLIENT	www.pepticoresaminos.net		

SAMPLE INFORMATION

Tirzepatide

10MG

FORM **White lyophilized powder in a glass vial**

SAMPLE SUBMISSION **Sample provided by customer**

BATCH **PC-TZ10-2012B**

CAP / CRIMP COLOR **blue/silver**

RECEIVED DATE **May 13, 2026**



SAMPLE IMAGE


ANALYTICAL SUMMARY

IDENTITY	Tirzepatide
PURITY	99.582%
QUANTITY	10.38mg
BATCH	PC-TZ10-2012B
MANUFACTURER	PepticoresAminos

RP-HPLC-UV CHROMATOGRAM (220 NM)

Detection: UV 220 nm | Runtime: 14.0 min

Sample ID: Tirzepatide
Report ID: 2024-02-01-000000
Method: RP-HPLC-UV Long Peptide
Detector: UV 220 nm | Runtime: 14.0 min

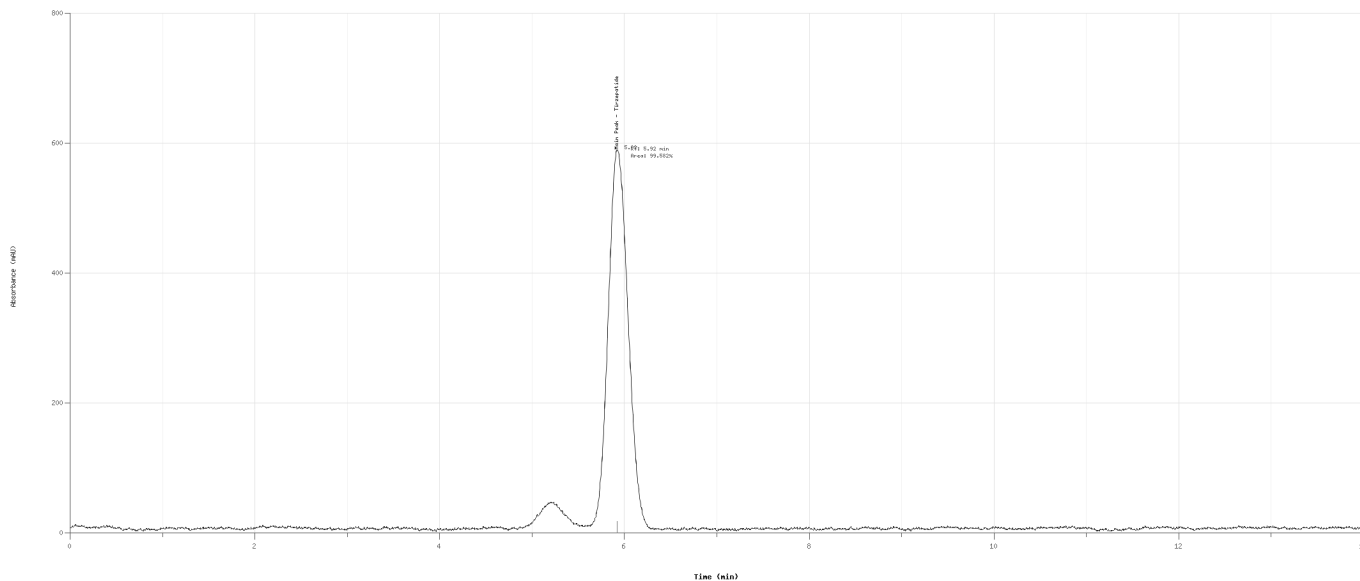

METHOD

TIME	H2O + 0.1% TFA	ACN + 0.1% TFA
0min	90%	10%
2min	90%	10%
10min	8%	92%
12min	8%	92%
14min	8%	92%

TECHNICAL NOTE

Analysis performed by RP-HPLC-UV at 220 nm using a gradient elution program. Total runtime: 14.0 minutes.


COMMENTS

The submitted sample meets the defined analytical specifications for identity, purity and impurity profile according to the applied RP-HPLC-UV method.

LC-MS MASS SPECTRUM

Sample: Tirzepatide
 Report ID: 278-2025-04069
 Reference MW: 4833.0 Da
 Ionization: ESI+

Acquisition: LC-MS
 Profile: Total Ion Chromatogram

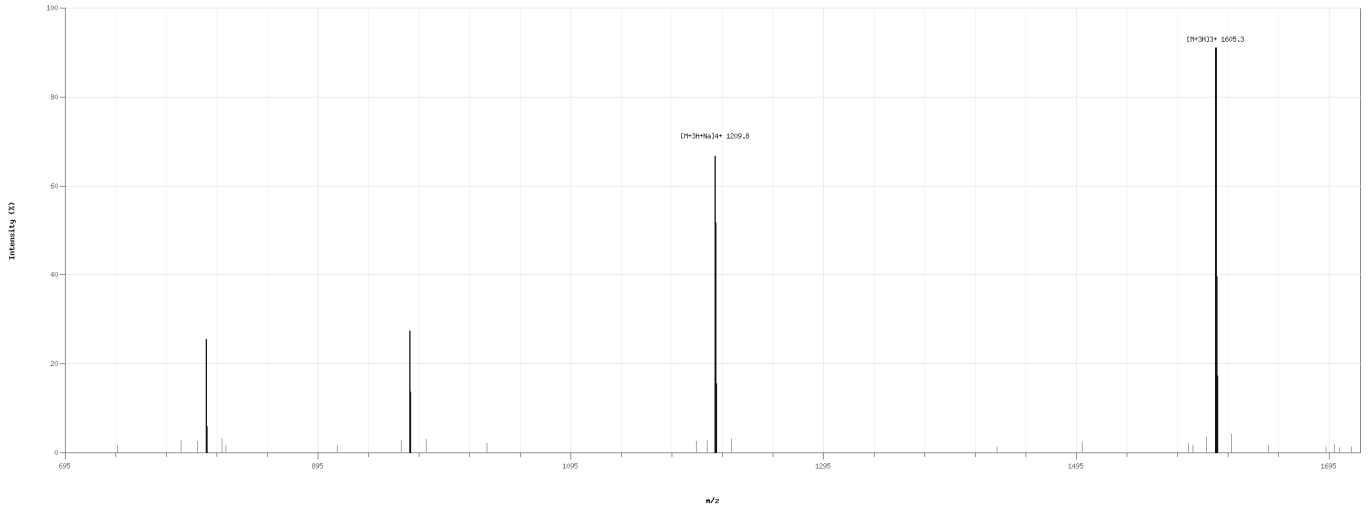

The recorded mass spectrum shows signals compatible with the expected molecular profile of the sample.

ANALYSIS & METHODOLOGY

STANDARD PEPTIDE PURITY, MASS & ADDITIONAL TESTING

Analysis performed using RP-HPLC-UV under validated laboratory conditions. Peak profile, retention behavior and purity response were evaluated against internal reference standards.

BIOBURDEN

TEST	RESULT	UNIT	REPORTING LIMIT
Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 1000
Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	Not detected	CFU/g	>= 100

ENDOTOXIN ANALYSIS

TEST	RESULT	UNIT	REPORTING LIMIT
Bacterial Endotoxin USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromogenic Test	< 0.001	EU/mg	> 0.5

HEAVY METALS

TEST	RESULT	UNIT	REPORTING LIMIT
Arsenic Elemental Impurities Screening	Not detected	ppm	>= 1.5
Cadmium Elemental Impurities Screening	Not detected	ppm	>= 0.5
Cobalt Elemental Impurities Screening	Not detected	ppm	>= 25
Lead Elemental Impurities Screening	Not detected	ppm	>= 1.5

TEST	RESULT	UNIT	REPORTING LIMIT
Nickel Elemental Impurities Screening	Not detected	ppm	>= 25
Quicksilver Elemental Impurities Screening	Not detected	ppm	>= 1.5
Vanadium Elemental Impurities Screening	Not detected	ppm	>= 25

TECHNICAL APPENDIX

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

COMPOUND REFERENCE

PARAMETER	TIRZEPATIDE
PUBCHEM CID	166567236
CAS	2023788-19-2
MOLECULAR FORMULA	C225H348N48O68
MOLECULAR WEIGHT	4813.0 g/mol

METHOD SPECIFICATION

PARAMETER	LONG PEPTIDE EXTENDED RP-HPLC-UV METHOD
ANALYTICAL MODE	Extended gradient RP-HPLC-UV peptide purity screen
COLUMN	C18 peptide column, extended-gradient configuration
MOBILE PHASE A	Water + 0.1% TFA
MOBILE PHASE B	Acetonitrile + 0.1% TFA
FLOW RATE	0.7 mL/min
DETECTION	UV 220 nm
INJECTION VOLUME	10 uL
RUNTIME	14.0 min
SAMPLE DILUENT	Water/acetonitrile compatible diluent
SAMPLE PREPARATION	Diluted to method range and clarified before injection

INSTRUMENT PLATFORM

PARAMETER	HIGH-RESOLUTION UPLC/HPLC-UV PLATFORM
SYSTEM TYPE	High-resolution LC platform
DETECTOR	UV/VIS detector
ACQUISITION	Chromatographic acquisition and integration software
REVIEW MODE	Gradient profile review with peak integration

PARAMETER	HIGH-RESOLUTION UPLC/HPLC-UV PLATFORM
WORKFLOW NOTE	Used for long peptide and multi-component profile review

ANALYTICAL CRITERIA

PARAMETER	ACCEPTANCE FRAMEWORK	BASIS
IDENTITY	Retention-time and profile agreement with reference expectations	Chromatographic identity review
PURITY	NLT 98.0% unless a stricter report-specific specification is declared	Integrated RP-HPLC-UV purity profile
QUANTITY	Measured content reviewed against the declared sample strength	Report-level analytical summary
BIOBURDEN	Not detected or within stated reporting limits	Microbial screening table
ENDOTOXIN	Below stated reporting limit / internal screening threshold	Endotoxin analysis table
HEAVY METALS	Below individual reporting limits where screened	Elemental impurities screening table

This appendix documents the analytical methodology, instrumentation and acceptance criteria applied for the evaluation of the sample.

VERIFICATION

Verify this report through the official Synaptica Analytics verification page using the details below.

Verification URL synaptica-labs.com/verify-report

Report ID SYN-2026-004989

Verification Key VK-PQ8S-D32W

SCAN TO VERIFY



DIGITAL SIGNATURE



DIGITALLY SIGNED BY:

Martin Saar

Date: 2026.05.19

09:54:22 +02'00'

Director

info@synaptica-labs.com

Analysis date: May 18, 2026

Report generated: May 19, 2026

Analytical testing performed by Synaptica Analytics -

Analytical Services Division

Synaptica Analytics
SYN-2026-004989
Laboratory Analysis Report
VK-PQ8S-D32W

VERIFY AT
synaptica-labs.com/verify-report